

AdipoGen[®] 
LIFE SCIENCES

MANUAL

Adiponectin (human) ELISA Kit

For research use only. Not for diagnostic use.

Version 3 (29-April-2015)

Cat. No. AG-45A-0001YEK-KI01

www.adipogen.com

Table of Contents

1. Intended Use	3
2. Introduction	3
3. General References	3
4. Assay Principle	4
5. Handling & Storage	4
6. Kit Components	4
7. Materials Required but <i>Not</i> Supplied	5
8. General ELISA Protocol	6
8.1. Preparation and Storage of Reagents	6
8.2. Sample Collection, Storage and Dilution	7
8.3. Assay Procedure (Checklist)	8
9. Calculation of Results	9
10. Typical Data	9
11. Performance Characteristics	10-12
12. Technical Hints and Limitations	13
13. Troubleshooting	14
14. Notes	15
Product Specific References	Backcover

1. Intended Use

The Adiponectin (human) ELISA Kit is to be used for the *in vitro* quantitative determination of human Adiponectin in serum, plasma, urine and cell culture supernatant. This ELISA Kit is for research use only.

2. Introduction

Adipocytes express a variety of adipocytokines that function in the homeostatic control of glucose and lipid metabolism. Insulin regulates secretion of many of these adipocytokines in response to changes in energy balance. Adiponectin is a 244-amino acid protein with high structural homology to collagen VIII, collagen V, complement C1q (Ref. 1 and 2), and TNF (Ref.3), which is exclusively and abundantly expressed in white adipose tissue. Plasma adiponectin concentrations have found to be decreased in obesity and/or type-2 diabetes, resulting in the conditions commonly associated with insulin resistance and hyper-insulinemia (Ref. 4-5). Therefore, measurement of the plasma level of adiponectin may be important for understanding diagnosis or prognosis of onset of these diseases.

3. General References

- (1) A novel serum protein similar to C1q, produced exclusively in adipocytes: P.E. Scherer, et al.; J. Biol. Chem. **270**, 26746 (1995)
- (2) AdipoQ is a novel adipose-specific gene dysregulated in obesity: E. Hu, et al.; J. Biol. Chem. **18**, 10697 (1996)
- (3) The crystal structure of a complement-1q family protein suggests an evolutionary link to tumor necrosis: L. Shapiro, et al.; Curr. Biol. **12**, 335 (1998)
- (4) Plasma resistin concentrations are elevated in Individuals with Type-2 diabetes mellitus: B.S. Youn, et al.; J. Cli. Endo. Meta. **89**, 150 (2004)
- (5) Genetic association study of adiponectin polymorphisms with risk of type 2 diabetes mellitus in Korean population: Y. Y. Lee, et al.; Diabet. Med. **22**, 569 (2004)

4. Assay Principle

This assay is a sandwich Enzyme Linked-Immunosorbent Assay (ELISA) for quantitative determination of human adiponectin in biological fluids. A monoclonal antibody specific for adiponectin has been precoated onto the 96-well microtiter plate. Standards and samples are pipetted into the wells for binding to the coated antibody. After extensive washing to remove unbound compounds, adiponectin is recognized by the addition of a purified polyclonal antibody specific for adiponectin (Detection Antibody). After removal of excess polyclonal antibody, HRP conjugated anti-rabbit IgG (HRP) is added. Following a final washing, peroxidase activity is quantified using the substrate 3,3',5,5'-tetramethylbenzidine (TMB). The intensity of the color reaction is measured at 450 nm after acidification and is directly proportional to the concentration of adiponectin in the samples.

5. Handling & Storage

- Reagent must be stored at 2-8°C when not in use.
- Plate and reagents should be at room temperature before use.
- Do not expose reagents to temperatures greater than 25°C.

6. Kit Components

1 plate coated with human Adiponectin Antibody	(6 x 16-well strips)	
2 bottles Wash Buffer 10X	(2 x 30 ml)	(Wash Buffer 10X)
2 bottles ELISA Buffer 10X	(2 x 30 ml)	(ELISA Buffer 10X)
1 vial Detection Antibody	(30 µl)	(DET)
1 vial HRP 100X (HRP Conjugated anti-rabbit IgG)	(150 µl)	(HRP 100X)
1 vial human Adiponectin Standard (lyophilized)	(64 ng)	(STD)
1 bottle TMB Substrate Solution	(12 ml)	(TMB)
1 bottle Stop Solution	(12 ml)	(STOP)
2 plate sealers (plastic film)		
2 silica Gel Minibags		

7. Materials Required but *Not* Supplied

- Microtiterplate reader at 450 nm
- Calibrated precision single and multi-channel pipettes. Disposable pipette tips
- Deionized water
- Microtubes or equivalent for preparing dilutions
- Disposable plastic containers for preparing working buffers
- Plate washer: automated or manual
- Glass or plastic tubes for diluting and aliquoting standard

8. General ELISA Protocol

8.1. Preparation and Storage of Reagents

NOTE: Prepare just the appropriate amount of the buffers necessary for the assay.

- **Wash Buffer 10X** has to be diluted with deionized water 1:10 before use (e.g. 50 ml Wash Buffer 10X + 450 ml water) to obtain Wash Buffer 1X.
- **ELISA Buffer 10X** has to be diluted with deionized water 1:10 before use (e.g. 20 ml ELISA Buffer 10X + 180 ml water) to obtain ELISA Buffer 1X.
- **Detection Antibody (DET)** has to be diluted to 1:1000 in ELISA Buffer 1X (10 µl DET + 10 ml ELISA Buffer 1X).

NOTE: The diluted Detection Antibody is not stable and cannot be stored!

- **HRP 100X (HRP Conjugated anti-rabbit IgG)** has to be diluted to the working concentration by adding 100 µl in 10 ml of ELISA Buffer 1X (1:100).

NOTE: The diluted HRP is used within one hour of preparation.

- **Human adiponectin Standard (STD)** has to be reconstituted with 1 ml of deionized water.
 - This reconstitution produces a stock solution of 64 ng/ml. Mix the standard to ensure complete reconstitution and allow the standard to sit for a minimum of 15 minutes. Mix well prior to making dilutions.

NOTE: The reconstituted standard is aliquoted and stored at -20°C.

- Dilute the standard protein concentrate (STD) (**64 ng/ml**) in ELISA Buffer 1X. A seven-point standard curve using 2-fold serial dilutions in ELISA Buffer 1X is recommended.
- Suggested standard points are:
32 , 16 , 8 , 4 , 2 , 1 , 0.5 and 0 ng/ml.

Dilute further for the standard curve:

To obtain	Add	Into
32 ng/ml	300 µl of adiponectin (64 ng/ml)	300 µl of ELISA Buffer 1X
16 ng/ml	300 µl of adiponectin (32 ng/ml)	300 µl of ELISA Buffer 1X
8 ng/ml	300 µl of adiponectin (16 ng/ml)	300 µl of ELISA Buffer 1X
4 ng/ml	300 µl of adiponectin (8 ng/ml)	300 µl of ELISA Buffer 1X
2 ng/ml	300 µl of adiponectin (4 ng/ml)	300 µl of ELISA Buffer 1X
1 ng/ml	300 µl of adiponectin (2 ng/ml)	300 µl of ELISA Buffer 1X
0.5 ng/ml	300 µl of adiponectin (1 ng/ml)	300 µl of ELISA Buffer 1X
0 ng/ml	300 µl of ELISA Buffer 1X	Empty tube

8.2. Sample Collection, Storage and Dilution

Serum : Use a serum separator tube. Let samples clot at room temperature for 30 minutes before centrifugation for 20 minutes at 1,000xg. Assay freshly prepared serum or store serum in aliquot at ≤ -20°C for later use. Avoid repeated freeze/thaw cycles.

Plasma : Collect plasma using heparin, EDTA, or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000xg within 30 minutes of collection. Assay freshly prepared plasma or store plasma sample in aliquot at ≤ -20°C for later use. Avoid repeated freeze/ thaw cycles.

Urine : Aseptically collect the urine of the day, voided directly into a sterile container. Assay immediately or aliquot and store at ≤ -20°C. Avoid repeated freeze/thaw cycles.

Serum, Plasma, Urine or Cell Culture Supernatant have to be diluted in ELISA Buffer 1X. Samples containing visible precipitates must be clarified before use.

NOTE: As a starting point, 1/2,000 dilution of serum or plasma and 1/10 dilution of urine are recommended! If sample values fall outside the detection range of the assay, a lower or higher dilution may be required!

8.3. Assay Procedure (Checklist)


<input type="checkbox"/>	<p>1. Determine the number of 16-well strips needed for the assay and insert them in the frame for current use. The extra strips should be resealed in the foil pouch bag and stored at 4°C.</p> <p>NOTE: Remaining 16-well strips coated with adiponectin antibody when opened can be stored at 4°C for up to 1 month.</p>
<input type="checkbox"/>	<p>2. Add 100 µl of the different standards into the appropriate wells in duplicate! At the same time, add 100 µl of diluted serum, plasma, urine or cell culture supernatant samples in duplicate to the wells (see 8.1. Preparation and Storage of Reagents and 8.2. Preparation of Samples).</p>
<input type="checkbox"/>	<p>3. Cover the plate with plate sealer and incubate for 1 hour at 37°C.</p>
<input type="checkbox"/>	<p>4. Aspirate the coated wells and add 300 µl of Wash Buffer 1X using a multichannel pipette or auto-washer. Repeat the process for a total of three washes. After the last wash, complete removal of liquid is essential for good performance.</p>
<input type="checkbox"/>	<p>5. Add 100 µl to each well of the Detection Antibody (DET). (see 8.1. Preparation and Storage of Reagents).</p>
<input type="checkbox"/>	<p>6. Cover the plate with plate sealer and incubate for 1 hour at 37°C.</p>
<input type="checkbox"/>	<p>7. Aspirate the coated wells and add 300 µl of Wash Buffer 1X using a multichannel pipette or auto-washer. Repeat the process for a total of three washes. After the last wash, complete removal of liquid is essential for good performance.</p>
<input type="checkbox"/>	<p>8. Add 100 µl to each well of the diluted HRP (see 8.1. Preparation and Storage of Reagents).</p>
<input type="checkbox"/>	<p>9. Cover the plate with plate sealer and incubate for 1 hour at 37°C.</p>
<input type="checkbox"/>	<p>10. Aspirate the coated wells and add 300 µl of Wash Buffer 1X using a multichannel pipette or auto-washer. Repeat the process for a total of five washes. After the last wash, complete removal of liquid is essential for good performance.</p>
<input type="checkbox"/>	<p>11. Add 100 µl to each well of TMB Substrate Solution (TMB).</p>
<input type="checkbox"/>	<p>12. Allow the color reaction to develop at room temperature (RT°C) in the dark for 20 minutes.</p>
<input type="checkbox"/>	<p>13. Stop the reaction by adding 100 µl of Stop Solution (STOP). Tap the plate gently to ensure thorough mixing. The substrate reaction yields a blue solution that turns yellow when Stop Solution (STOP) is added.</p>
	<p>! CAUTION: CORROSIVE SOLUTION!</p>
<input type="checkbox"/>	<p>14. Measure the OD at 450 nm in an ELISA reader within 30 minutes.</p>

9. Calculation of Results

- Average the duplicate readings for each standard, control and sample and subtract the average blank value (obtained with the 0 ng/ml point).
- Generate the standard curve by plotting the average absorbance obtained for each standard concentration on the horizontal (X) axis vs. the corresponding adiponectin concentration (ng/ml) on the vertical (Y) axis (see **10. TYPICAL DATA**).
- Calculate the adiponectin concentrations of samples by interpolation of the regression curve formula as shown above in a form of a quadratic equation.
- If the test samples were diluted, multiply the interpolated values by the dilution factor to calculate the concentration of human adiponectin in the samples.

10. Typical Data

The following data are obtained using the different concentrations of standard as described in this protocol:

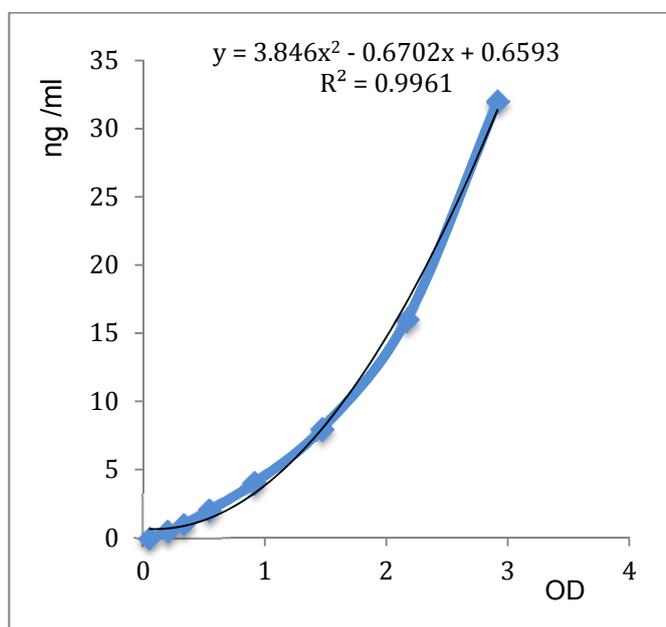

Standard hAdiponectin (ng/ml)	Optical Density (mean)
32	2.863
16	2.1165
8	1.417
4	0.861
2	0.488
1	0.2795
0.5	0.151
0	0

Figure: Standard curve

11. Performance Characteristics

A. Sensitivity (Limit of detection):

The lowest level of adiponectin that can be detected by this assay is 100 pg/ml. **NOTE:** *The Limit of detection was measured by adding two standard deviations to the mean value of 50 zero standard.*

B. Assay range: 0.5 ng/ml – 32 ng/ml

C. Specificity:

This ELISA is specific for the measurement of natural and recombinant human adiponectin. It does not cross-react with mouse adiponectin, rat adiponectin, human resistin, human RELM- β , human leptin, human TNF- α , human IL-6.

D. Intra-assay precision:

Four serum samples of known concentrations of human adiponectin were assayed in replicates 5 times to test precision within an assay.

Samples	Means (μ g/ml)	SD	CV (%)	n
1	1.86	0.07	3.82	5
2	5.90	0.23	3.84	5
3	8.50	0.28	3.31	5
4	23.36	0.69	2.97	5

Five urine samples of known concentrations of human adiponectin were assayed in replicates 6 times to test precision within an assay.

Samples	Means (ng/ml)	SD	CV (%)	n
1	30.40	2.53	8.31	6
2	5.42	0.41	7.54	6
3	10.28	0.34	3.33	6
4	95.83	3.38	3.53	6
5	69.94	1.48	2.12	6

E. Inter-assay precision:

Four serum samples of known concentrations of human adiponectin were assayed in 5 separate assays to test precision between assays.

Samples	Means (µg/ml)	SD	CV (%)	n
1	2.50	0.13	5.15	5
2	7.78	0.43	5.50	5
3	11.10	0.44	3.97	5
4	24.82	0.70	2.84	5

Five urine samples of known concentrations of human adiponectin were assayed in 3 separate assays to test precision between assays.

Samples	Means (ng/ml)	SD	CV (%)	n
1	28.16	1.81	6.44	3
2	5.94	0.23	3.93	3
3	3.91	0.36	9.09	3
4	108.91	8.26	7.58	3
5	76.13	7.38	9.69	3

F. Recovery:

The recovery of adiponectin spiked to four different levels in five different serum samples and four different urine samples throughout the range of assay was evaluated.

Samples	Average recovery (%)	Range (%)	
Serum	1	99.6	96-105
	2	99.8	96-104
	3	100.2	97-102
	4	92.5	88-95
	5	91.8	86-100
Urine	1	101.9	96-105
	2	97.9	96-104
	3	91.2	88-95
	4	84.7	80-90

G. Linearity:

Different human serum samples containing adiponectin were diluted several fold (1/1,000 to 1/4,000) and the measured recoveries ranged from 87% to 102%.

Samples	Sample Dilution	Expected (µg/ml)	Observed (µg/ml)	% of Expected
1	1 : 1,000	13.61	13.61	100
	1 : 2,000	6.81	6.64	97.6
	1 : 4,000	3.40	2.97	87.2
2	1 : 1,000	15.89	15.89	100
	1 : 2,000	7.94	8.09	101.9
	1 : 4,000	3.97	3.76	94.7
3	1 : 1,000	11.51	11.51	100
	1 : 2,000	5.76	5.77	100.2
	1 : 4,000	2.88	2.51	87.1

Different human urine samples containing adiponectin were diluted several fold (1/5 to 1/10) and the measured recoveries ranged from 97% to 105%.

Samples	Sample Dilution	Expected (ng/ml)	Observed (ng/ml)	% of Expected
1	1 : 5	3.85	3.85	100
	1 : 10	1.92	2.00	104.2
2	1 : 5	5.14	5.14	100
	1 : 10	2.57	2.66	103.8
3	1 : 5	45.79	45.79	100
	1 : 10	22.89	23.56	102.9

H. Expected values:

Adiponectin levels range in plasma and serum from **4 to > 15 µg/ml** (from healthy donors).

Adiponectin levels range in urine from **3 to > 15 ng/ml** (from healthy donors).


12. Technical Hints and Limitations

- It is recommended that all standards, controls and samples be run in duplicate.
- Do not combine leftover reagents with those reserved for additional wells.
- Reagents from the kit with a volume less than 100 µl should be centrifuged.
- Residual wash liquid should be drained from the wells after last wash by tapping the plate on absorbent paper.
- Crystals could appear in the 10X solution due to high salt concentration in the stock solutions. Crystals are readily dissolved at room temperature or at 37°C before dilution of the buffer solutions.
- Once reagents have been added to the 16-well strips, DO NOT let the strips DRY at any time during the assay.
- Keep TMB Substrate Solution (TMB) protected from light.
- The Stop Solution (STOP) consists of sulfuric acid. Although diluted, the Stop Solution (STOP) should be handled with gloves, eye protection and protective clothing.

13. Troubleshooting

PROBLEM	POSSIBLE CAUSES	SOLUTIONS
No signal or weak signal	Omission of key reagent	Check that all reagents have been added in the correct order.
	Washes too stringent	Use an automated plate washer if possible.
	Incubation times inadequate	Incubation times should be followed as indicated in the manual.
	Plate reader settings not optimal	Verify the wavelength and filter setting in the plate reader.
	Incorrect assay temperature	Use recommended incubation temperature. Bring substrates to room temperature before use.
High background	Concentration of HRP too high	Use recommended dilution factor.
	Inadequate washing	Ensure all wells are filling wash buffer and are aspirated completely.
Poor standard curve	Wells not completely aspirated	Completely aspirate wells between steps.
	Reagents poorly mixed	Be sure that reagents are thoroughly mixed.
Unexpected results	Omission of reagents	Be sure that reagents were prepared correctly and added in the correct order.
	Dilution error	Check pipetting technique and double-check calculations.

14. Notes

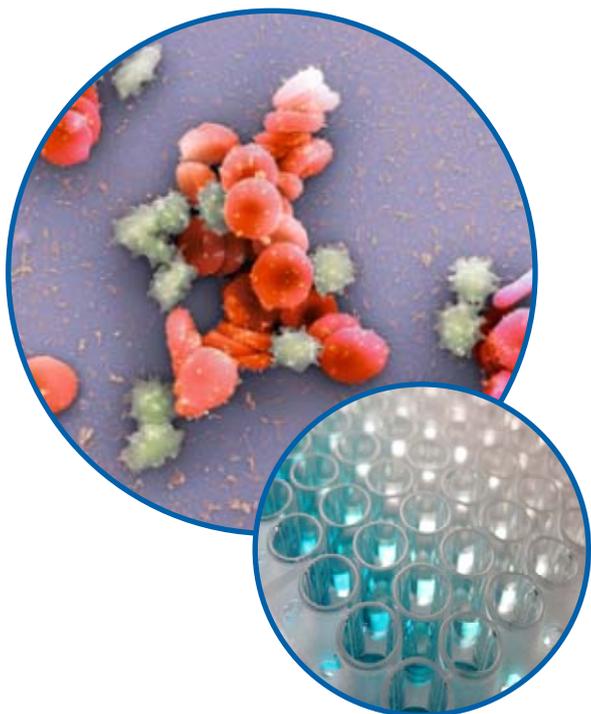

Product Specific References:

1. J.A. Im, et al.; Metabol. Clin. Exp. **55**, 1546 (2006)
2. T. Yasui, et al.; Clinica. Chimica. Acta. **386**, 69 (2007)
3. E.S. Kim, et al.; Obesity (Silver Spring) **15**, 3023 (2007)
4. S. Lim, et al.; J. Clin. Endocrinol. Metab. **93**, 2263 (2008)
5. S. Lim, et al.; Obesity (Silver Spring) **17**, 188 (2009)
6. A. Tonjes, et al.; PLoS One **5**, e13911 (2010)
7. S.W. Oh, et al.; Breast Cancer Res. **13**, R34 (2011)
8. H.G. Jeong, et al.; Psychoneuroendocrinol. **37**, 948 (2012)
9. W.S. Jeon, et al.; Cardiovasc. Diabetol. **12**, 137 (2013)

For more References please visit www.adipogen.com!

Adipogen Life Sciences
Schützenstrasse 12
CH-1410 Liestal
Switzerland
TEL: +41-61-926-60-40
FAX: +41-61-926-60-49
Email: info@adipogen.com

AdipoGen[®] 

LIFE SCIENCES